

▶ Tr1 S12 Log Mag 1.000dB/ Ref 0.000dB

E5062A Menu

Measurement

S12

Format

Log Mag

Scale

Display


Average

Calibration

Stimulus

Sweep Setup

Trigger

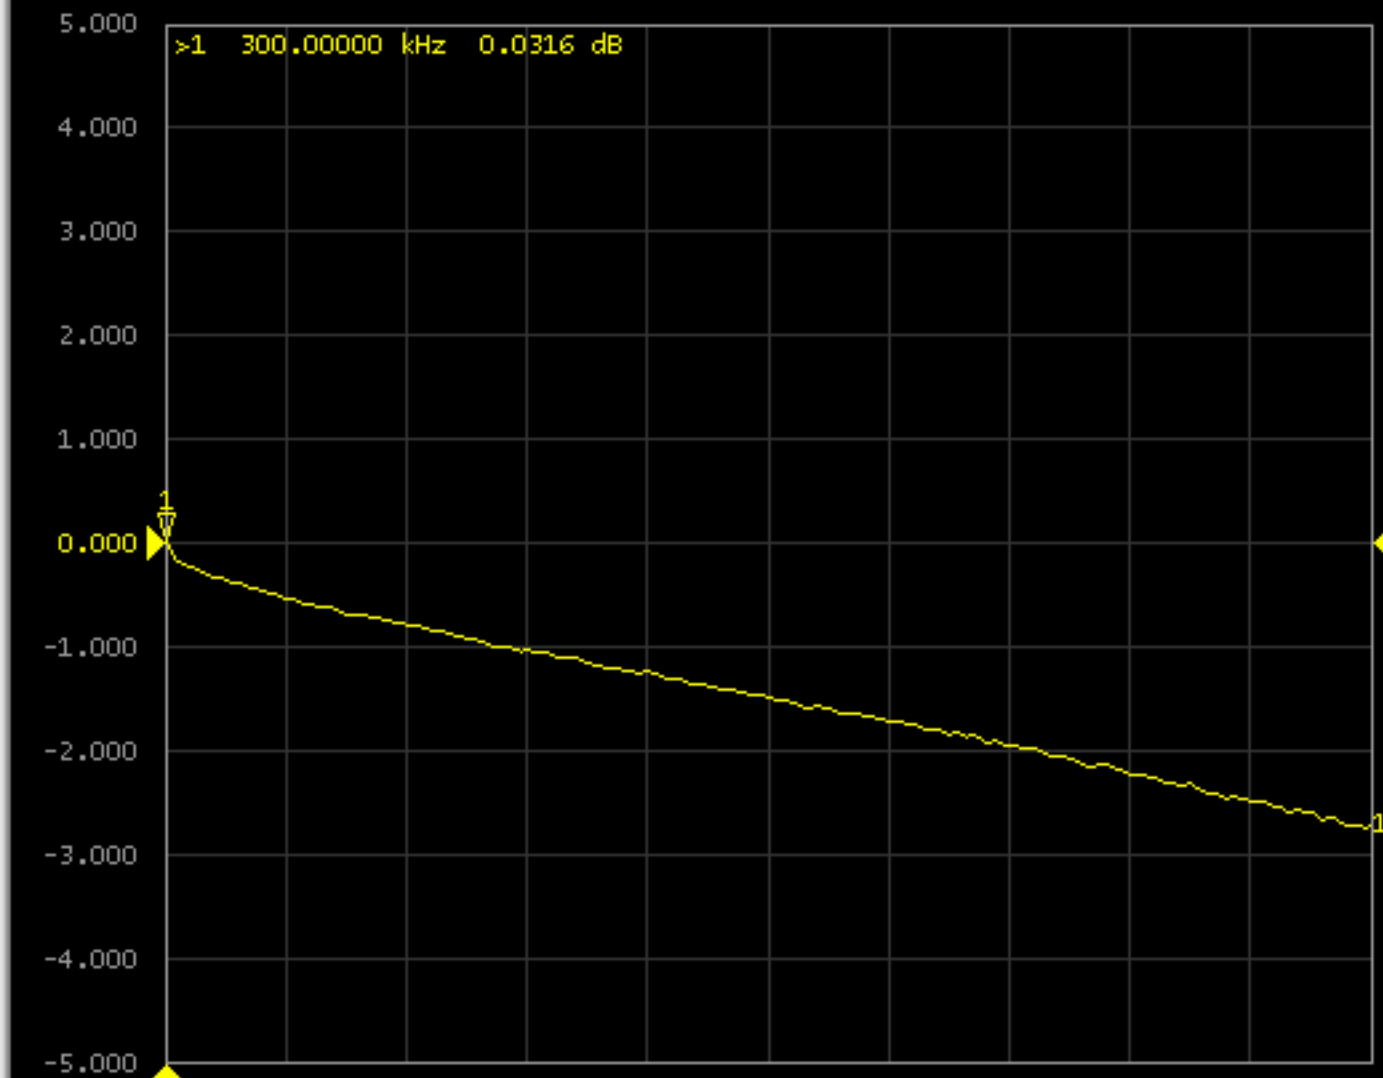

1 Start 300 kHz

IFBW 30 kHz

Stop 3 GHz

Meas

Stop

ExtRef

Svc

2008-12-09 20:22